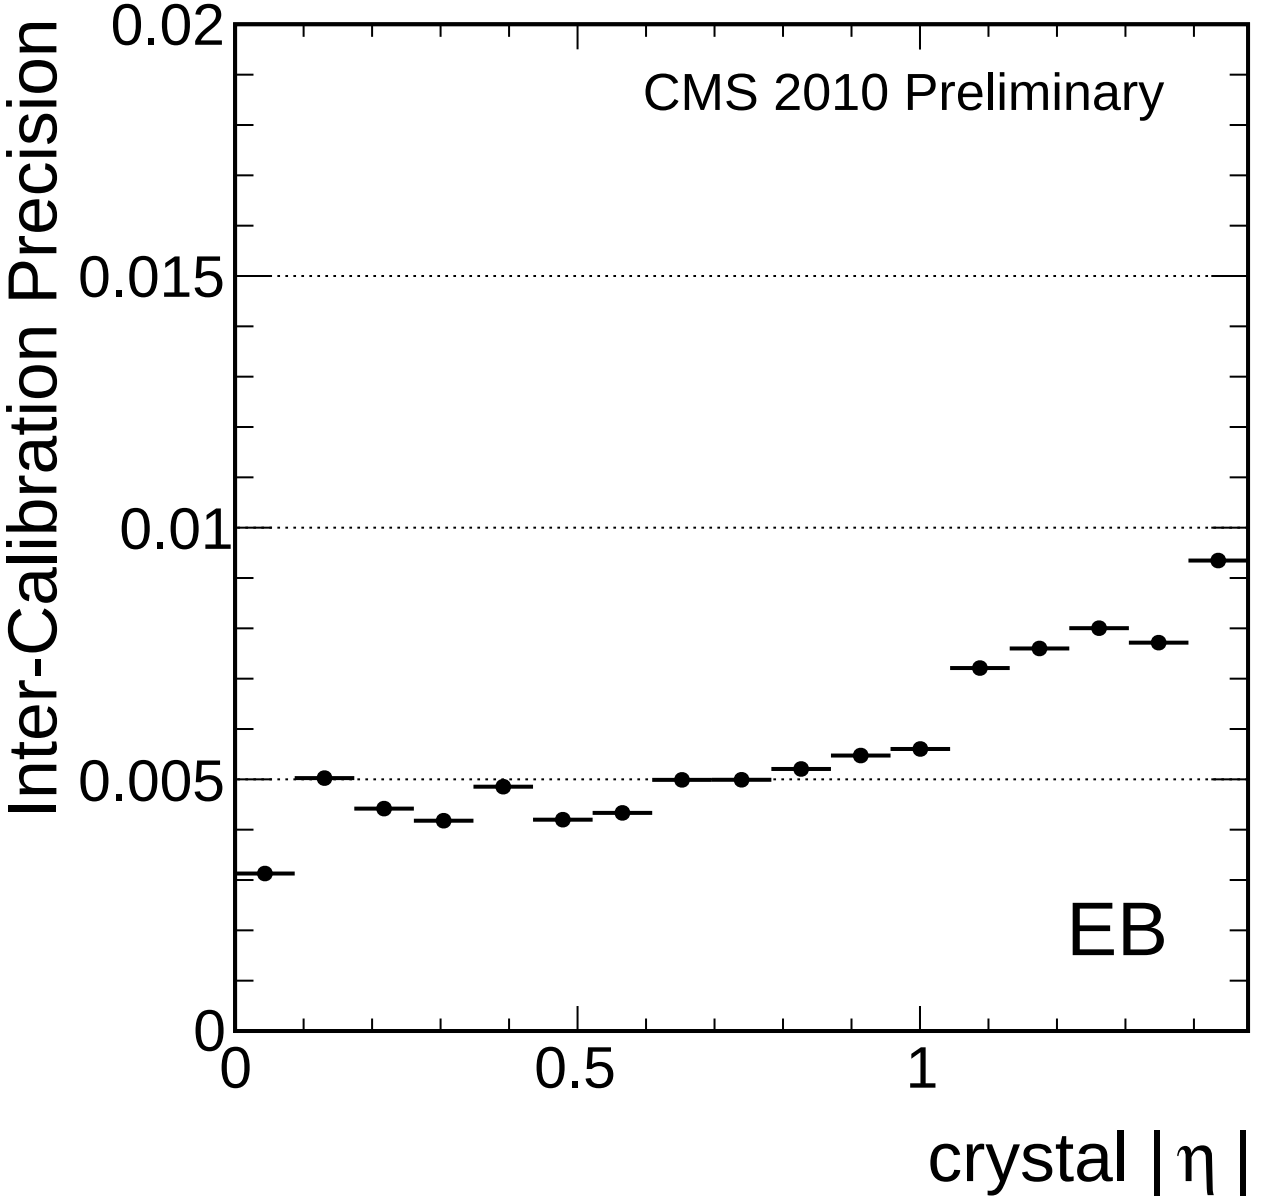
CMS 2010 Preliminary
EB
Inter-Calibration Precision
0.02
0.015
0.01
0.005
0
0
0.5
1
crystal | η |